


RBR Temperature Calibration Certificate

Logger ID: RBRconcerto Serial No: 66030 Channel No: 2

Reference Temperature, ITS-90	Voltage ratio, V	Measured Temperature, ITS-90	Calibration error	Coefficients
-4.97765	0.723277	-4.97760	0.00005	C0: 0.003482990960063
0.66722	0.659825	0.66710	-0.00012	C1: -0.000253520092968
6.89271	0.585525	6.89277	0.00005	C2: 0.000002509808573
12.80001	0.513916	12.80002	0.00001	C3: -0.000000068344474
18.56767	0.445841	18.56777	0.00010	
24.31446	0.382135	24.31439	-0.00007	
30.10911	0.323686	30.10901	-0.00010	
34.99510	0.279588	34.99517	0.00008	

Residuals vs. Temperature

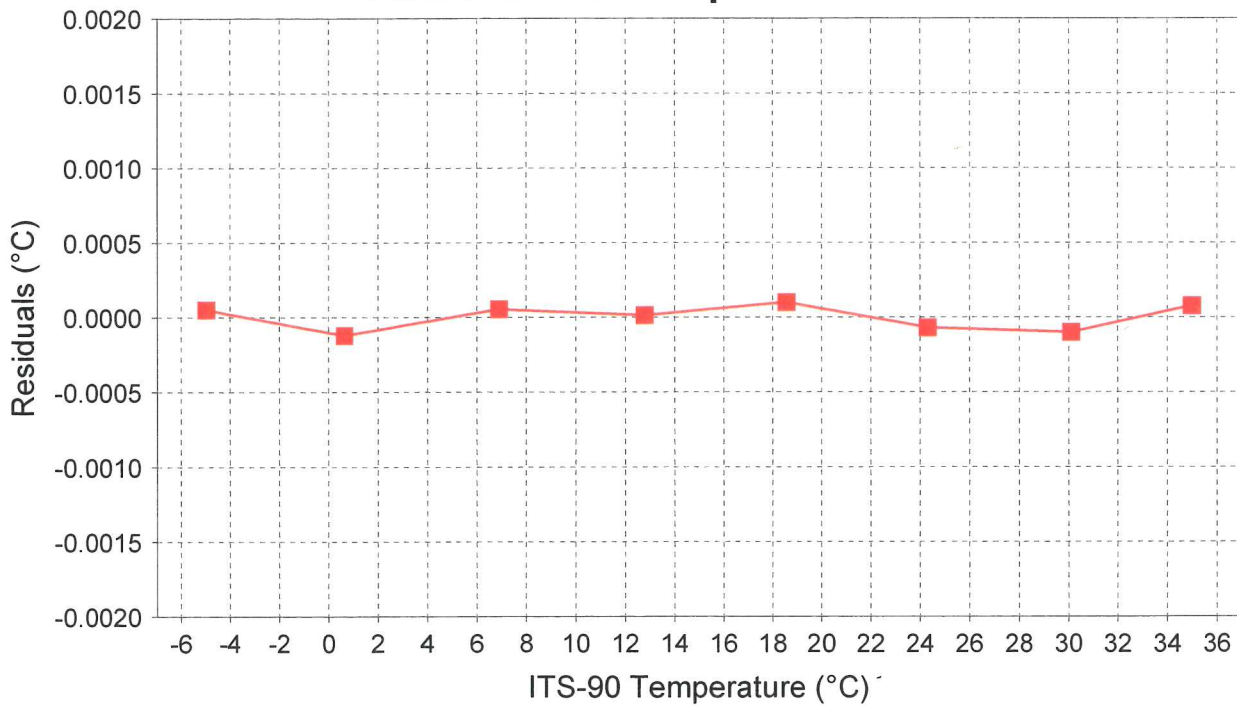

Calibration Date: 8/Mar/2017
Issue Date: 9/Mar/2017
Calibration ID: 19204

Operator: 
tjenkins

Approver: 
sbucknor